


Calibration of flow meters

In the CS calibration laboratory for flow meters it is possible to calibrate our flow measuring instruments as well as of other manufacturers High precision reference measuring devices guarantee an accuracy of up 0.5% of the measured value.

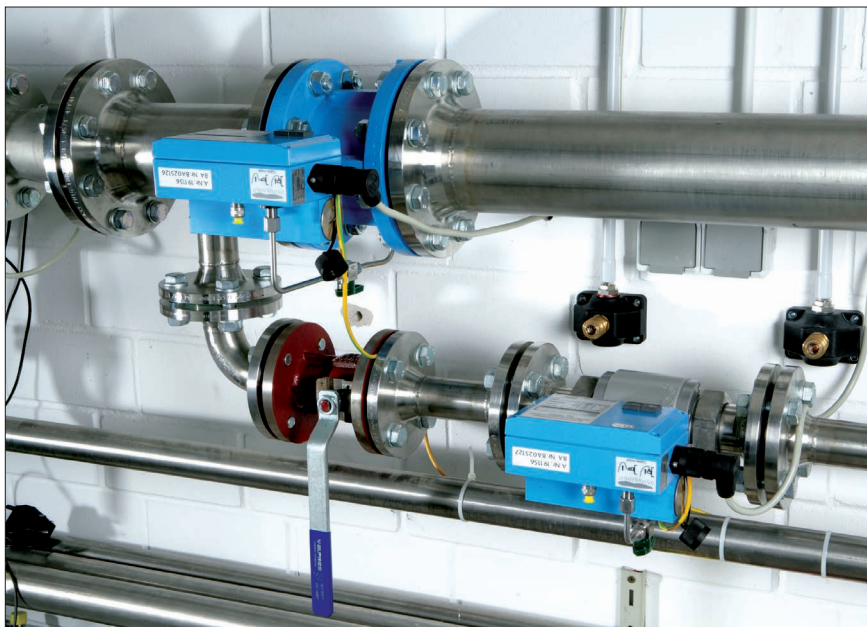

Special features:

- Due to the digital data transmission, only the flow meter must be calibrated. The display devices remain wired on site.

| | |
|-----------------------------------|--|
| Calibration range: | from 0 to 4.000 m ³ /h under pressure |
| Accuracy of the reference: | between 0.5 and 1% of the measured value |

| DESCRIPTION | ORDER NO. |
|--|------------|
| Recalibration and 5 point precision calibration of volume flow sensors VA 500/550 with ISO certificate | 0695 3333 |
| Recalibration and 5 point precision calibration of volume flow sensors VA 520/570 with ISO certificate | 0695 3332 |
| Volume flow, any measuring points | on request |
| Real gas adjustment | 3200 0015 |